

LIME WA INC.
Independently Audited
Lime Suppliers

SERVING AGRICULTURE FOR 20 YEARS

Tel: 9757 6263
Mob: 0407 385 488
admin@redgatelime.com.au
566 Redgate Rd, Redgate WA 6286



Tested by a
Code of Practice
Approved Laboratory



PRODUCT INFORMATION SHEET

GENERAL INFORMATION			
PIT NAME	Redgate Lime	DATE	December 17th 2019
LOCATION	Witchcliffe	LIME WA REF. LAB NO.	B1912-0167
DESCRIPTION	Limestone	SCREENED SCREEN SIZE	Yes 10.0mm
WEIGH SYSTEM	Compuload Loader Scales [Accredited weigh system verified by Trade Measurement Services]		

CODE OF PRACTICE APPROVED LABORATORY REPORT				
SIEVE RANGE (MM)	% WEIGHT		% NEUTRALISING VALUE	
	THIS TEST	3 YEAR PIT RANGE	THIS TEST	3 YEAR PIT RANGE
0.000 - 0.125	1.4	1.4 : 2.2	92.3	92.3 : 93.7
0.125 - 0.250	19.3	19.3 : 24.1	94.8	94.8 : 96.8
0.250 - 0.500	43.7	43.7 : 45.6	94.6	94.6 : 96.8
0.500 - 1.000	23.9	23.9 : 24.6	91.4	91.4 : 93.2
> 1.000	11.8	3.5 : 11.8	92.6	87.8 : 92.6
CALCIUM (1M HCL)	35.6	35.5 : 35.6		
MAGNESIUM (1M HCL)	1.3	1.2 : 1.3		
SODIUM (1M HCL)	0.1	0.1 : 0.1		
			WEIGHTED AVE NV	93.6 93.6 : 95.5
			BULK NV	93.4 93.4 : 94.8

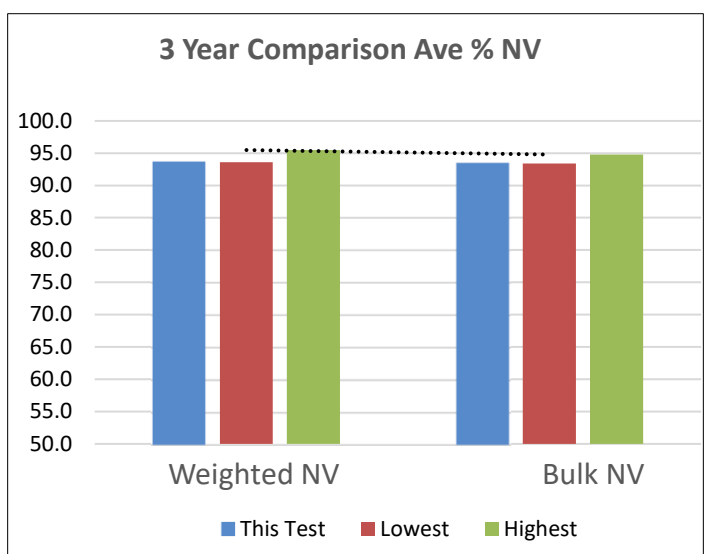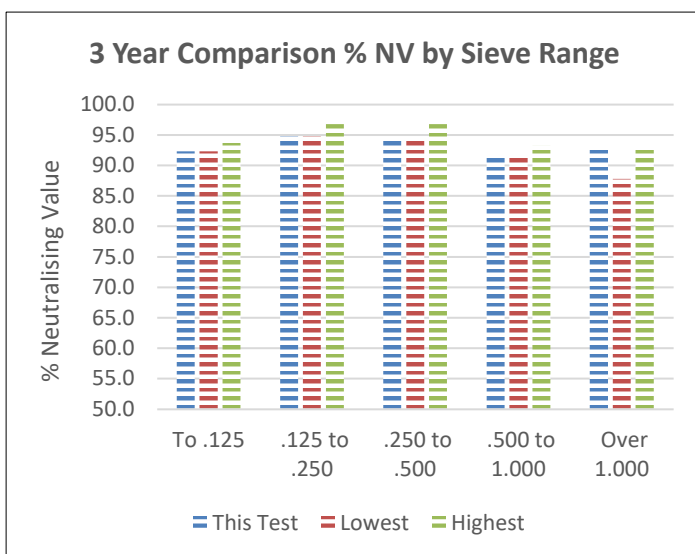

DISCLAIMER & SUPPLIER STATEMENT : The supplier states that the above analysis, provided by a Lime WA Inc Agricultural Lime Industry Code of Practice approved laboratory, is a true representation of the product being supplied. However, this test is for one lime sample collected on one day. The pit ranges show results obtained within the past three years, but please contact your supplier for analyses over a longer timeframe. Lime WA Inc requires members to provide the above details in accordance with the Code of Practice requirements, but makes no claims and provides no guarantees on the quality or suitability of the product supplied. Product supplied by members occurs naturally and has a moisture retention capacity that varies according to seasonal conditions. As this cannot be controlled by suppliers, moisture levels are not stated. Lime WA Inc is not responsible for any claims and/or liabilities arising from the supply and/or use of these products. However, lime users are invited to contact the Association on 0419 575 737 in the event of any dissatisfaction with the product details provided by